



Using LOGGER for Food Temperature Monitoring

USER MANUAL

DRAGONNORTH GROUP

Using LOGGER for Food Temperature Monitoring
User Manual

1 Contents

1	Contents.....	1
2	Introduction	3
3	Network Setup	4
3.1	Tell LOGGER About Your Network Server	4
3.1.1	Connect to the LOGGER	4
3.1.2	Talk to the Logger With a Web Browser.....	5
3.1.3	Network Setup Page.....	6
3.1.4	Enter SSID Name and SSID Password	7
3.1.5	Network Setup Complete	8
3.1.6	Optional: Name Your LOGGER	9
4	Temperature History.....	10
5	Names for Food	13
6	Sampling and Logging Strategy	15
7	Identifying Sensors.....	16
7.1	Default Temperature Sensor Names	16
7.2	User Defined Names	17
8	Software Updates	18
9	Additional Sensors	19
9.1	Analog to Digital conversion.	19
9.2	Digital Inputs and Outputs.	19
9.2.1	Temperature and Humidity or Temperature Humidity and Atmospheric Pressure.	19
9.3	Water Flow Measurement	19
9.4	Power Consumption Measurement	21
10	Future Capabilities	22
10.1	Text Alerts	22
11	Advanced Features	23
11.1	Choosing Engineering Units	23
11.1.1	Centigrade vs Fahrenheit	23
11.2	Database Control	24
11.3	Email Alerts	26
11.3.1	Set up SMTP Server	26



Using LOGGER for Food Temperature Monitoring
User Manual

11.3.2	Set Sensor Limits	27
11.4	Battery Operation	28
11.6	Security	29
11.7	Exporting Data	29
12	Time Synchronization.....	31
13	Data Storage	31
14	Troubleshooting.....	33
14.1	Missing Database	33
14.2	Can Not See the LOGGER	33




Using LOGGER for Food Temperature Monitoring

User Manual

2 Introduction

For food monitoring the LOGGER typically is used to record a history of temperatures. Other sensors if connected are also logged. The LOGGER reads sensors and creates a permanent record of what it has observed. This data is stored on the SD card inserted into the LOGGER. By default, the LOGGER reads all sensors every 10 seconds. A 32Gb card will store at least 20 years of data.

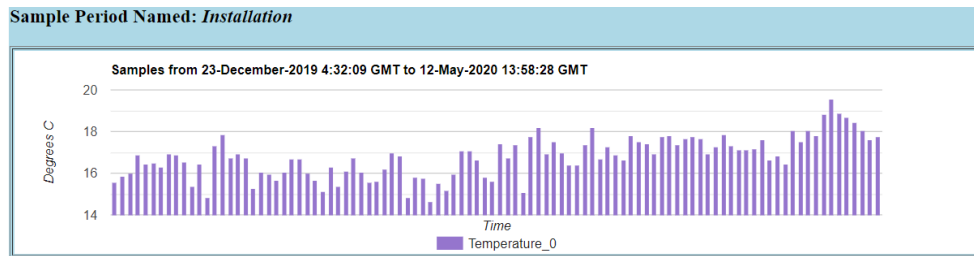

The LOGGER is a miniature Web Server allowing you the user to observe the history and control the LOGGER from tablets, computers and smart phones.

The LOGGER presents on it's web pages a menu of choices which allow the user to navigate among options. Sections of this menu will be covered in later chapters of this document.



Caution: The connectors on the LOGGER box are the same connectors that are used for the internet. These connectors are not internet connections and should not be plugged in to your router. The LOGGER communicates only by WiFi.



3 Network Setup


When the LOGGER is first turned on it is ready to work with you. In addition to being a Web Server the LOGGER is an Access Point (like a WiFi router). You can connect to the LOGGER as you do with any WiFi router and then use it as a Web Server. After connecting to the LOGGER all of the LOGGER web pages are available. Connect to the LOGGER as if it were a WiFi router and browse to <http://10.1.1.1/>. Some display features (graphs in particular) will not work when you use the LOGGER as your Access Point (Wifi router). These features depend on libraries that your browser must obtain from servers on the internet. When you use the LOGGER as an Access Point the rest of the internet is not available.

3.1 Tell LOGGER About Your Network Server


The LOGGER does not know about your local WiFi network when you start. To tell it about the local network first connect to it instead of the local network. The images below come from a Windows computer. Tablets, Smart Phones or Apple computers will not exactly match.

3.1.1 Connect to the LOGGER

Scan the local WiFi networks on your phone or tablet. The LOGGER shows up in the list of networks using the name LOGGER_xxxx where xxxx is part of the LOGGER's serial number.

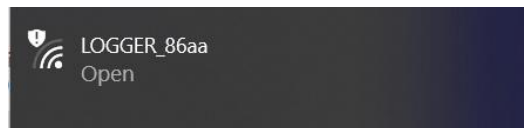


Treat the LOGGER like any other WiFi network and connect to it. The Tablet or Computer system will likely say that there is “No Internet”. This is normal, while connected to the LOGGER you will only be able to see the LOGGER itself and will not be able to browse other web sites.

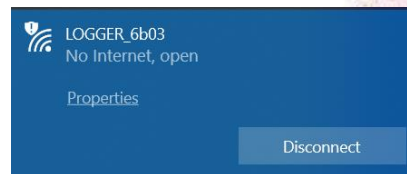

Using LOGGER for Food Temperature Monitoring User Manual

3.1.2 Talk to the Logger With a Web Browser

Open a web browser and type <http://10.1.1.1/> into the address line browser. This will bring up the home page of the LOGGER showing the Current Sensor Values:

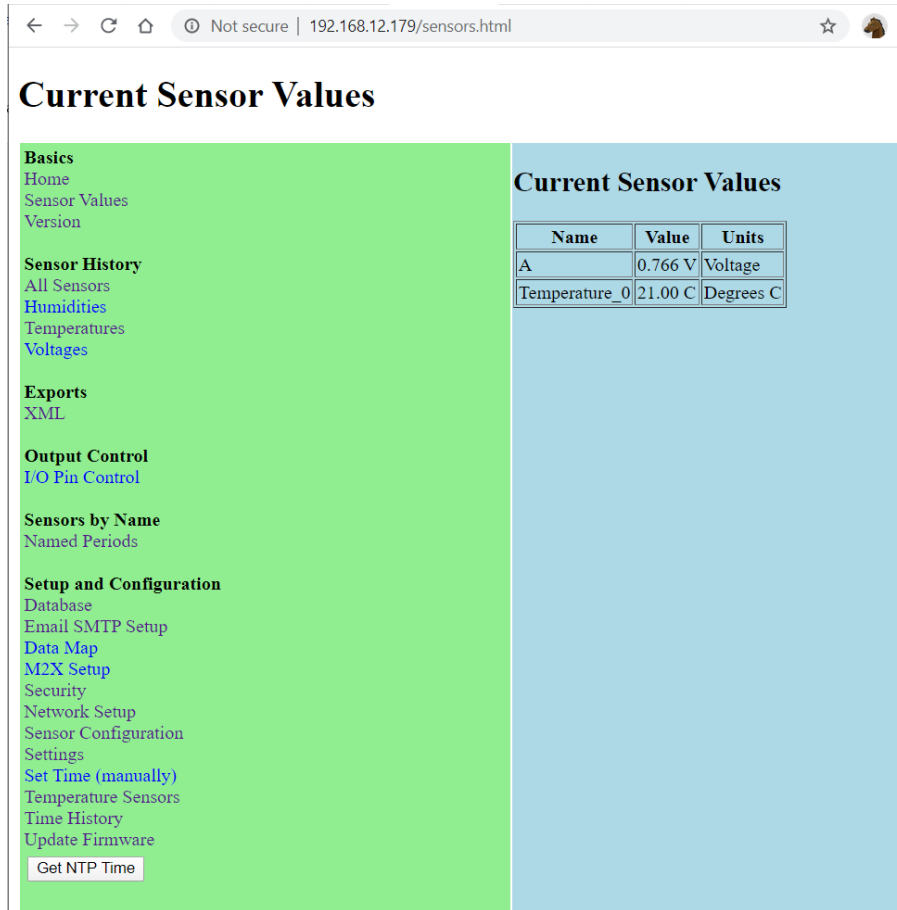

Current Sensor Values

Basics
[Home](#)
[Sensor Values](#)
[Version](#)

Sensor History
[All Sensors](#)
[Humidities](#)
[Temperatures](#)
[Voltages](#)

Exports
[XML](#)

Output Control
[I/O Pin Control](#)

Sensors by Name
[Named Periods](#)

Setup and Configuration
[Database](#)
[Email SMTP Setup](#)
[Data Map](#)
[M2X Setup](#)
[Security](#)
[Network Setup](#)
[Sensor Configuration](#)
[Settings](#)
[Set Time \(manually\)](#)
[Temperature Sensors](#)
[Time History](#)
[Update Firmware](#)
[Get NTP Time](#)

Current Sensor Values


Name	Value	Units
A	0.766 V	Voltage
Temperature_0	21.00 C	Degrees C



Using LOGGER for Food Temperature Monitoring User Manual

3.1.3 Network Setup Page

Choose “Network Setup” from the menu at the left



to bring up the Network Configuration page:

A screenshot of the "Network Configuration" page. The page has a light blue background and contains the following sections:

- Network Configuration**
 - Available Networks**

FJQNK	-89	*
KudosDen	-66	*
Kudos-Guest	-73	
LOGGER_6b03	-69	
KudosDen	-73	*
Kudos-Guest	-47	
KudosDen	-47	*
Kudos-Guest	-66	
 - Primary Network SSID**
(max 32characters)
SSID_NAME
 - Password for WEP/WPA/WPA2**
(enter a space if there is no password, i.e. OPEN)
(max 32 characters)
SSID_PASSWORD
 -

Using LOGGER for Food Temperature Monitoring User Manual

3.1.4 Enter SSID Name and SSID Password

In the SSID_NAME field enter the name of your wireless router and press the **Set** button next to that field.



Network Configuration

Available Networks

FJQNK	-89 *
KudosDen	-66 *
Kudos-Guest	-73
LOGGER_6b03	-69
KudosDen	-73 *
Kudos-Guest	-47
KudosDen	-47 *
Kudos-Guest	-66

Primary Network SSID
(max 32characters)

SSID_NAME Wireless **Set**

Password for WEP/WPA/WPA2
(enter a space if there is no password, i.e. OPEN)
(max 32 characters)

SSID_PASSWORD password **Set**

Reboot

It is very important to press the **Set** button before going on to the next step.

Next enter the password of your wireless router where it says SSID_PASSWORD and press that **Set** button.



Network Configuration

Available Networks

FJQNK	-89 *
KudosDen	-66 *
Kudos-Guest	-73
LOGGER_6b03	-69
KudosDen	-73 *
Kudos-Guest	-47
KudosDen	-47 *
Kudos-Guest	-66

Primary Network SSID
(max 32characters)

SSID_NAME Wireless **Set**

Password for WEP/WPA/WPA2
(enter a space if there is no password, i.e. OPEN)
(max 32 characters)


SSID_PASSWORD password **Set**

Reboot



Using LOGGER for Food Temperature Monitoring User Manual

Finally press the **Reboot** button. Don't forget to press the **Set** button for the password first.

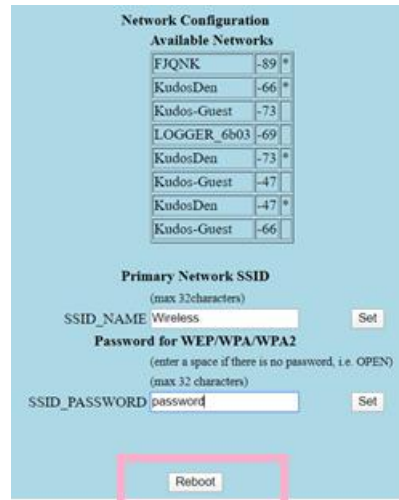

Available Networks	
FJQNK	-89 *
KudosDen	-66 *
Kudos-Guest	-73
LOGGER_6b03	-69
KudosDen	-73 *
Kudos-Guest	-47
KudosDen	-47 *
Kudos-Guest	-66

Primary Network SSID
(max 32 characters)


SSID_NAME: Wireless Set

Password for WEP/WPA/WPA2
(enter a space if there is no password, i.e. OPEN)
(max 32 characters)

SSID_PASSWORD: password Set


Reboot

After pressing the **Reboot** button it will likely be necessary to connect to the LOGGER WiFi network again. It can take a minute for the system to reboot. After connecting to the LOGGER WiFi network again browse to <http://10.1.1.1/>.



Basics
Home
Sensor Values
Version

At the bottom of the menu System Status information is displayed. Write down the Local IP address (192.168.12.179 is shown here yours will be different). This address will be needed later:

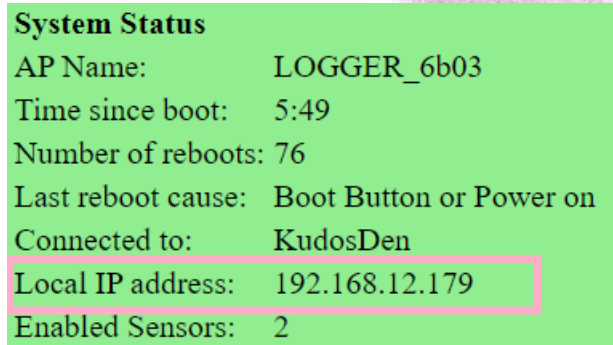

System Status

AP Name: LOGGER_6b03

Time since boot: 5:49

Number of reboots: 76

Last reboot cause: Boot Button or Power on

Connected to: KudosDen

Local IP address: 192.168.12.179

Enabled Sensors: 2



3.1.5 Network Setup Complete


LOGGER network setup is now complete, reconnect to your normal WiFi network.



Using LOGGER for Food Temperature Monitoring User Manual


3.1.6 Optional: Name Your LOGGER

Like a WiFi router the LOGGER has a name that shows up in the list of WiFi routers. This name starts out as LOGGER_xxxx where xxxx comes from the unique MAC address of the LOGGER (green box below). you can change this name. Call the logger whatever you want “Refrigerator_7” might be a good name for the LOGGER watching that refrigerator. Fill in your desired name (pink box) and press the  button. Remember the name will change, the LOGGER will now use this name (in your WiFi router list) after a .

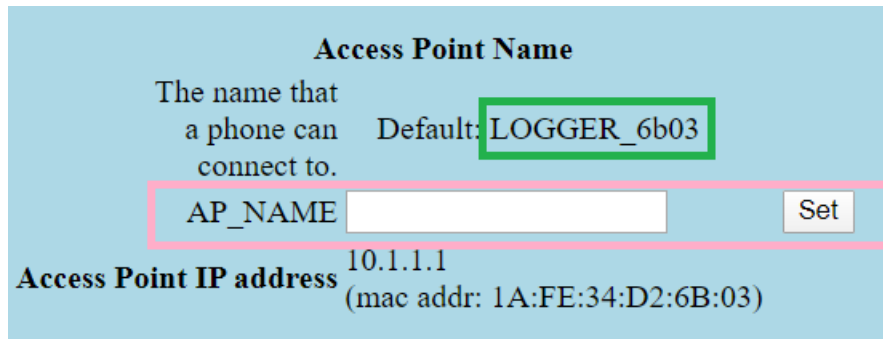

Access Point Name

The name that a phone can connect to. Default: **LOGGER_6b03**

AP_NAME 

Access Point IP address 10.1.1.1
(mac addr: 1A:FE:34:D2:6B:03)



Using LOGGER for Food Temperature Monitoring User Manual

4 Temperature History

Put the **Local IP address** noted when the system was set up into your browser. This brings up a page on the LOGGER acting as a web server.

Click on **Temperatures** in the menu to get this page.

Sensor History

Basics
Home
Sensor Values
Version

Sensor History
All Sensors
Humidities
Temperatures
Voltages

Exports
XML

Output Control
I/O Pin Control

Sensors by Name
Named Periods

Setup and Configuration
Database
Email SMTP Setup
Data Map
M2X Setup
Security
Network Setup
Sensor Configuration
Settings
Set Time (manually)
Temperature Sensors
Time History
Update Firmware
Get NTP Time

System Status
AP Name: LOGGER_6b03
Time since boot: 8:54
Number of reboots: 76
Last reboot cause: Boot Button or Power on
Connected to: KudosDen
Local IP address: 192.168.12.179
Enabled Sensors: 2

Latest samples for the same interval: Most Recent 20:00

Adjust Times to Get the Latest Samples: Hour Day Week Month Quarter Year

Move time window: << One Day >>

Adjust Columns to: No Change Update

Datatype to display: Degrees C Update

Sensor to display: All Sensors Update

Manually Change the Interval
Starting (GMT): 13-May-2020 13:29:14
Ending (GMT): 13-May-2020 13:49:14
Columns in the graph: 15 (0:01:20 per column)
Lines in the table: 10
Update Graph and Table

Samples from 13-May-2020 13:29:14 GMT to 13-May-2020 13:49:14 GMT

Time	Element
13-May-2020 13:49:14 GMT	Temperature_0 = 18.31 C
13-May-2020 13:47:54 GMT (data logged at 13-May-2020 13:47:14 GMT)	Temperature_0 = 18.37 C
13-May-2020 13:46:34 GMT (data logged at 13-May-2020 13:45:14 GMT)	Temperature_0 = 18.50 C
13-May-2020 13:45:14 GMT	Temperature_0 = 18.50 C
13-May-2020 13:43:54 GMT (data logged at 13-May-2020 13:43:14 GMT)	Temperature_0 = 18.50 C
13-May-2020 13:42:34 GMT (data logged at 13-May-2020 13:41:14 GMT)	Temperature_0 = 18.37 C
13-May-2020 13:41:14 GMT	Temperature_0 = 18.37 C
13-May-2020 13:39:54 GMT (data logged at 13-May-2020 13:39:14 GMT)	Temperature_0 = 18.37 C
13-May-2020 13:38:34 GMT (data logged at 13-May-2020 13:37:14 GMT)	Temperature_0 = 18.31 C
13-May-2020 13:37:14 GMT	Temperature_0 = 18.31 C
13-May-2020 13:35:54 GMT (data logged at 13-May-2020 13:35:14 GMT)	Temperature_0 = 18.25 C
...more samples exist...	

Current Time: 13-May-2020 13:49:52 GMT
Configuration is: OK from database
Database starts at: 3-May-2020 1:05:14 GMT
Database ends at: 13-May-2020 13:49:14 GMT
Last Sample: 13-May-2020 13:49:14 GMT
Next Sample Due: 13-May-2020 13:51:14 GMT

LOGGER Copyright (c) 2015-2020 by Dragonnorth Group
portions Copyright (c) 2014-2020 by Michael Newman (DBA Dragonnorth Group)
all rights reserved
LOGGER version 1(72)-186 Processor module Serial Number: 0
built with ARDUINO version 10812


The section of the page outlined in black is the Menu. There are a number of headings in the menu that group the menu items by their purpose. Clicking on the **Temperatures** link brought up this page. The example page has only one temperature sensor. Your system may have several temperature sensors

Below the menu is system status information.



Using LOGGER for Food Temperature Monitoring User Manual

This Section of the page allows you to select what you are seeing in the graph and table below it.

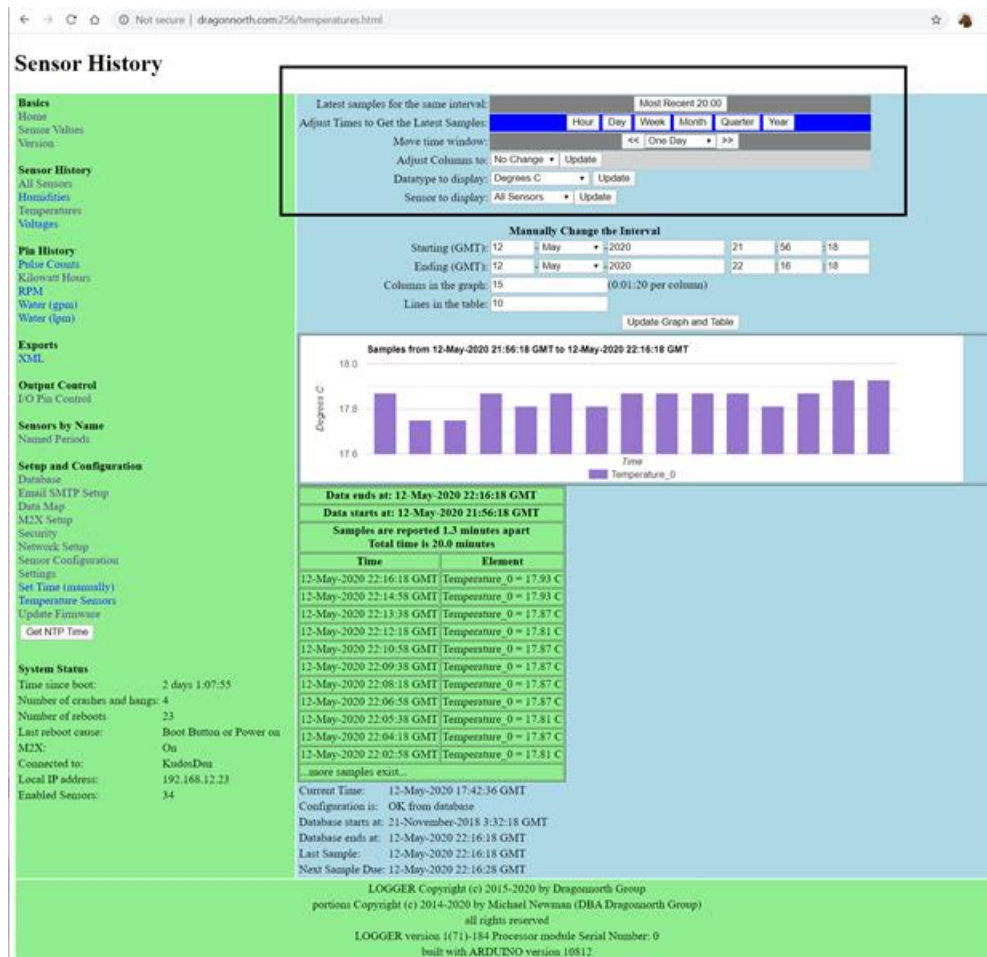

To keep this discussion simple, pull down the “Sensor to Display” field, choose Temperature_0 and press the Update button next to that field.

This image is a close-up of the 'Sensor to display' control in the Logger web interface. It shows a dropdown menu with 'All Sensors' selected. The 'Update' button next to the dropdown is highlighted with a red box. The other controls in the 'Latest samples for the same interval:' section are also visible, including the 'Adjust Times to Get the Latest Samples:' dropdown (set to 'Hour'), the 'Move time window:' dropdown (set to 'One Day'), the 'Adjust Columns to:' dropdown (set to 'No Change'), the 'Datatype to display:' dropdown (set to 'Degrees C'), and the 'Sensor to display:' dropdown (set to 'All Sensors').



Using LOGGER for Food Temperature Monitoring User Manual

The next section of the page shows what is currently being displayed in the graph and table below it.

The graph shows temperature readings over the selected time period. The table shows some of these readings. You control how many readings are in the table by adjusting the “Lines in the table:” field.

Date time and columns are all user selectable fields. Change any of the fields and then click the update button to refresh the display.

Basic

Home

Sensor Values

Version

Sensor History

All Sensors

Humidities

Temperatures

Voltages

Pin History

Pulse Counts

Kilowatt Hours

RPM

Water (gpm)

Water (lpm)

Exports

XML

Output Control

I/O Pin Control

Sensors by Name

Named Periods

Setup and Configuration

Database

Email SMTP Setup

Data Map

M2X Setup

Security

Network Setup

Sensor Configuration

Settings

Set Time (manually)

Temperature Sensors

Update Firmware

Get NTP Time

System Status

Time since boot:

2 days 1:07:55

Number of crashes and hangs:

4

Number of reboots:

23

Last reboot cause:

Boot Button or Power on

M2X:

On

Connected to:

KudosDen

Local IP address:

192.168.12.23

Enabled Sensors:

34

Latest samples for the same interval: Most Recent 20:00

Adjust Times to Get the Latest Samples: Hour Day Week Month Quarter Year

Move time window: << One Day >>

Adjust Columns to: No Change Update

Datatype to display: Degrees C Update

Sensor to display: All Sensors Update

Manually Change the Interval

Starting (GMT): 12 May 2020 21:56:18

Ending (GMT): 12 May 2020 22:16:18

Columns in the graph: 15 (0:01:20 per column)

Lines in the table: 10

Update Graph and Table

Samples from 12-May-2020 21:56:18 GMT to 12-May-2020 22:16:18 GMT

Degrees C

18.0

17.8

17.6

Time

Temperature_0

Data ends at: 12-May-2020 22:16:18 GMT

Data starts at: 12-May-2020 21:56:18 GMT

Samples are reported 1.3 minutes apart

Total time is 20.0 minutes

Time	Element
12-May-2020 22:16:18 GMT	Temperature_0 = 17.93 C
12-May-2020 22:14:58 GMT	Temperature_0 = 17.93 C
12-May-2020 22:13:38 GMT	Temperature_0 = 17.87 C
12-May-2020 22:12:18 GMT	Temperature_0 = 17.81 C
12-May-2020 22:10:58 GMT	Temperature_0 = 17.87 C
12-May-2020 22:09:38 GMT	Temperature_0 = 17.87 C
12-May-2020 22:08:18 GMT	Temperature_0 = 17.87 C
12-May-2020 22:06:58 GMT	Temperature_0 = 17.87 C
12-May-2020 22:05:38 GMT	Temperature_0 = 17.81 C
12-May-2020 22:04:18 GMT	Temperature_0 = 17.87 C
12-May-2020 22:02:58 GMT	Temperature_0 = 17.81 C
...more samples exist...	

Current Time: 12-May-2020 17:42:36 GMT

Configuration is: OK from database

Database starts at: 21-November-2018 3:32:18 GMT

Database ends at: 12-May-2020 22:16:18 GMT

Last Sample: 12-May-2020 22:16:18 GMT

Next Sample Due: 12-May-2020 22:16:28 GMT

LOGGER Copyright (c) 2015-2020 by Dragonnorth Group

portions Copyright (c) 2014-2020 by Michael Newman (DBA Dragonnorth Group)

all rights reserved

LOGGER version 1(71)-184 Processor module Serial Number: 0

built with ARDUINO version 10812

Dragonnorth Group

LOGGER release 1(73) or Later

Page 12

5 Names for Food

Keeping a log of food temperatures is a key feature of the LOGGER. Food sellers are required to keep temperature logs when food is stored (cold chain), when dishes are transported for delivery or sale and even sometimes when dishes are displayed for sale.

The LOGGER has a special feature to support this recordkeeping called Named Periods. A container of food is assembled for the Cotwell Party. When a LOGGER is placed in that container the Display Name is set and the Start Named Period button is pressed. The LOGGER now remembers when data collection started for that delivery and the record can be read by pressing the Cotwell Party Delivery button. When the LOGGER is used for another purpose the next Named Period is started and the knowledge of when the Cotwell Party Delivery ended is recorded.

Named Periods

Basics

[Home](#)

[Sensor Values](#)

[Version](#)

Sensor History

[All Sensors](#)

[Humidities](#)

[Temperatures](#)

[Voltages](#)

Exports

[XML](#)

Output Control

[I/O Pin Control](#)

Sensors by Name

[Named Periods](#)

When a Named Period is started it is given a name. Clicking on the button for that name will display the sensor values from the start of that Named Period until the next time a Named Period is created for that sensor. Names can be reused. The most recent Named Period created for a sensor continues collecting data until a new Named Period is created.

Start New Named Period

Sensor	Display Name	
Temperature_0 ▾	<input type="text"/>	Start Named Period

Named Periods To Display

Period Name	Sensor	End Time	Start Time
Cotwell Party Delivery	Temperature_0	Now	12-May-2020 21:37:32 GMT




Using LOGGER for Food Temperature Monitoring User Manual

Clicking one of the Period Name buttons:

Period Name	Sensor	End Time	Start Time
Cotwell Party Delivery	Temperature_0	Now	12-May-2020 21:37:32 GMT
Temp 0	Temperature_0	12-May-2020 21:37:32 GMT	7-March-2020 3:27:10 GMT

brings up the temperature history for that period.

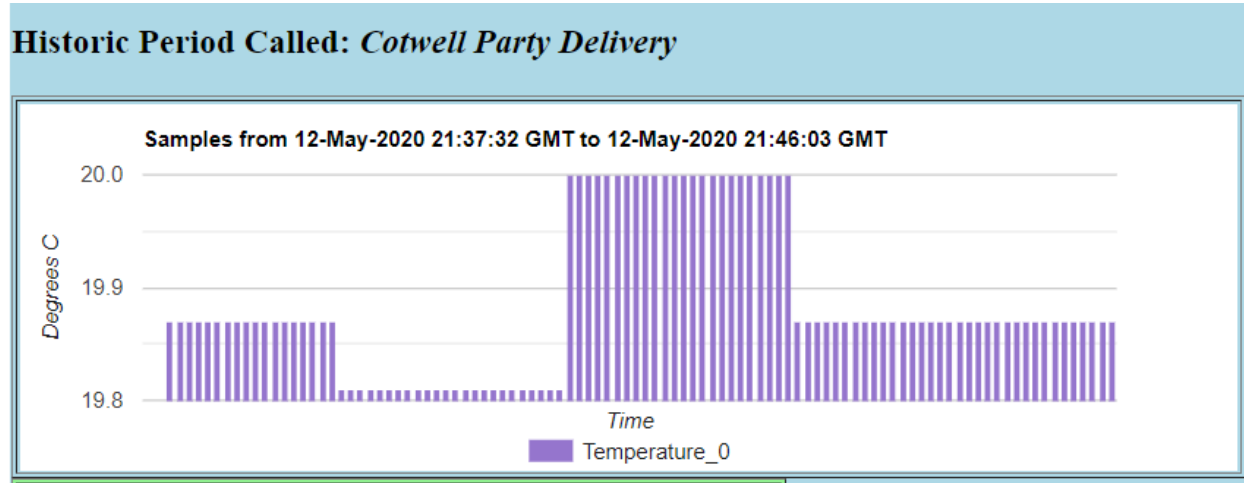

Should someone get sick after the party it is always easy to return to the history and prove that the food was kept at a proper temperature.



6 Sampling and Logging Strategy

Sensors are read and the values are appended to the log every sampling period (10 second default). The data recorded each sampling period is a fixed size, always the same size. Finding an element at a particular time is just going to the correct place in the log file. This is much faster than a database search and makes the LOGGER possible on a tiny inexpensive processor.

This also means that the amount of time it takes to display 100 elements is the same no matter what date and time those elements come from.

The strategy of logging every sample period is especially important when recording liquid flow or kilowatt hours. Each of these are measured by a counter that counts an exact number of times per gallon (or kWh). The count keeps going up all the time. What is logged in the data file is the current value of the counter. If you want to know how many gallons were used between 12:05 and 1:33 read the counts for each of those times and subtract! Keeping counts of usage to date makes knowing how much was used in any interval possible and makes the display of the usage data independent of the time period. Report on how much was used each day or every 13 minutes without any difficulty and no performance difference. The time period of the summary period is chosen at the time of display, NOT the time of data logging.



7 Identifying Sensors

7.1 Default Temperature Sensor Names

The temperature sensors used by the LOGGER are OneWire devices and each sensor has a unique serial number. The LOGGER remembers these devices and gives each of them a name. The same sensor will always be given the same name. This map of names can be erased. The LOGGER will give the sensors names in the order it sees the sensors. To start over type ERASE in the field and then press the Erase Map button. Then power off the LOGGER and unplug all of the temperature sensors. Power the LOGGER on and the on-board temperature sensor will be found and called Temperature_0. Power the LOGGER off and plug in the next temperature sensor. Power it on and that will become Temperature_1. Do this one at a time and all of the sensors get names that are known.

← → ↻ 🏠 ⓘ Not secure | 192.168.12.179/onewiresetup.html ☆ 🔔 ⋮

Temperature Sensors

Basics
Home
Sensor Values
Version

Sensor History
All Sensors
Humidities
Temperatures
Voltages

Exports
XML

Output Control
I/O Pin Control

Sensors by Name
Named Periods

Setup and Configuration
Database
Email SMTP Setup
Data Map
M2X Setup
Security
Network Setup
Sensor Configuration
Settings
Set Time (manually)
Temperature Sensors
Time History
Update Firmware
Get NTP Time

Onewire Temperature Sensors

Temperature_0	103a80530208007b
Temperature_1	0000000000000000
Temperature_2	0000000000000000
Temperature_3	0000000000000000
Temperature_4	0000000000000000
Temperature_5	0000000000000000
Temperature_6	0000000000000000
Temperature_7	0000000000000000

The above map of Onewire temperature sensors is kept so a sensor will always use the same name and will always show up in the same place in the database. The map can fill up and prevent sensors from being added even though one was physically removed. Erasing this map will cause confusion in the sensor history. The map between sensor names and database entries will be different so the temperature history for a particular name will come from a different sensor.

Erasing is usually a bad idea. If you need to make a change after the erase refreshes the page and confirms success unplug all of the temperature sensors and reboot the system. Wait a long time to make sure the system starts and finds the processor board temperature sensor. The best method is to wait until you can bring up the Sensors web page and see the sensor. The temperature sensor on the processor board will then be Temperature_0. Plug in another temperature sensor and reboot the system again. This sensor will become Temperature_1. Be sure and wait a long time again. Repeat for each temperature sensor.

After adding all of the sensors it is a good idea to discard the database and start over. This can be done on the [Database Page](#).

Input 'ERASE' and press the button to erase the map.

Erase Map

Reboot

7.2 User Defined Names

It is also possible to create your own names to replace the LOGGER's default names. Any sensor can be given a user defined name, not just temperature sensors. User defined names are created on the Sensor Configuration page. Put your own name in the field under the New Name column (blue box). Click the

Set New Name

button. The LOGGER will start using your name instead of the system default name (green box) on this page and on all other pages. The user defined names are recorded in a file called `usersensornames.bin` on the LOGGER's SD card. It is possible to erase all of the user defined

names and revert to the default names. Input ERASE in the box and press the

Erase User Sensor Names

button. Although the user sensor names are forgotten this will not change until the LOGGER is restarted. This can be done by pressing the

Reboot

Basics

Home

Sensor Values

Version

Sensor History

All Sensors

Humidities

Temperatures

Voltages

Exports

XML

Output Control

I/O Pin Control

Sensors by Name

Named Periods

Setup and Configuration

Database

Email SMTP Setup

Data Map

M2X Setup

Security

Network Setup

Sensor Configuration

Settings

Set Time (manually)

Temperature Sensors

Time History

Update Firmware

Get NTP Time

System Status

WiFi

Name: LOGGER_6b03

Time

since 8:07:38

boot:

Number

of reboots: 111

Sensor Configuration

Alerts are sent by text and/or email when the sensor value is less than the minimum or greater than the maximum. Set both to 0 to turn off alerts.

Each time the name of a sensor is changed (Set New Name) the time and new name is logged. At system startup this list is read and the most recent name is used.

Name	Information	Settings
A	0.666 V Uses 12 bits Unique ID: 1afe34d26b030000 Device: Processor ADC pin Datatype: Voltage 3 decimal places Sensor specific data: 17	<input type="text"/> Set New Name Min Max 0.000 0.000 Set New Limits
Temperature_0	25.18 C Uses 16 bits Unique ID: 103a80530208007b Device: DS18x20 Datatype: Degrees C 2 decimal places Sensor specific data: 0	<input type="text"/> Set New Name Min Max 0.00 10.00 Set New Limits

96 sensors (124 allowed) with 94 disabled. 95 bytes (754 bits) of sensor data.

0 Set Time Between Alerts

When a value goes out of range an email and/or text is sent. To prevent a great number of alerts from being sent once an alert is sent additional alerts will not be sent for this period.
A value of 0 turns off email alerts.

Erase User Sensor Names

Input 'ERASE' and click the button to clear the user defined sensor names.
Pressing this button will erase the entire history of user name setting. A reboot is necessary to revert to the default names.

Erase Email and Alerts


Input 'ERASE' and click the button to clear the Min/Max alerts.
Pressing this button will erase the entire history of alerts. A reboot is necessary to eliminate all alerts.


Reboot



8 Software Updates

Software updates are downloaded from the dragonnorth.com server. Sourcing the update from a local computer is not allowed for security reasons. To update the LOGGER firmware to the latest version

simply go to the Update Firmware page and click on the  button.

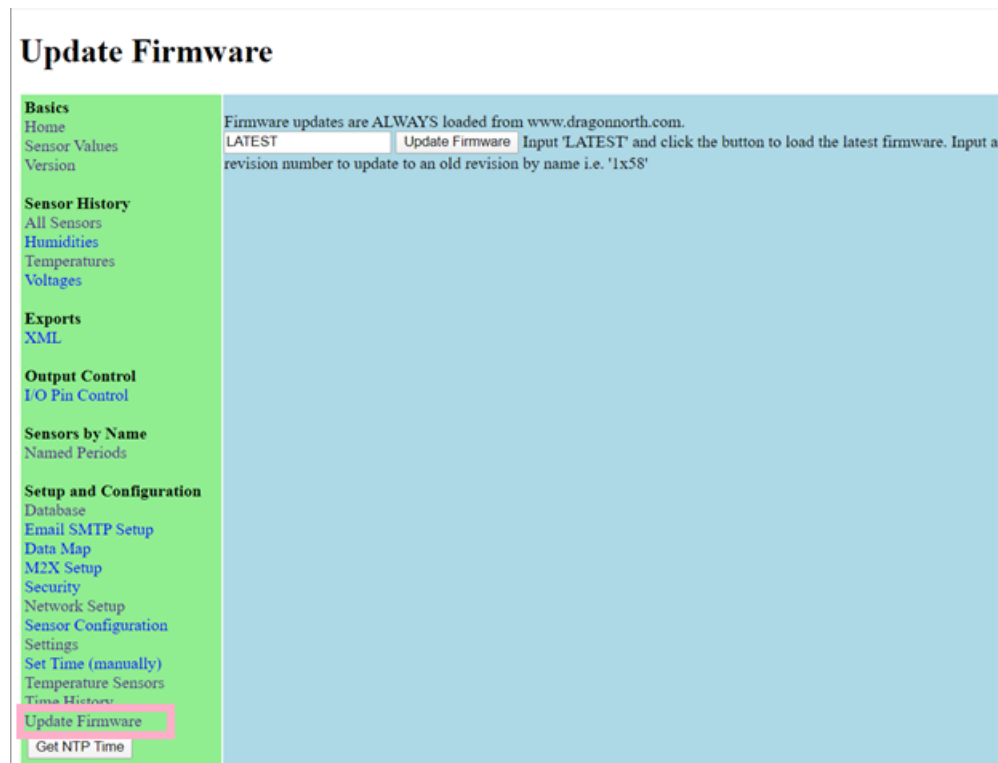

A poor network connection or congestion between the LOGGER being updated and the **dragonnorth.com** server can result in a failure in the update process. These failures are not easily noticed except by checking that the version number of the software has been properly updated.

Updates are safe, an update failure will not damage a LOGGER. When an update fails the LOGGER simply continues to run the old software.



9 Additional Sensors

The LOGGER understands many additional sensors. These sensors come in separate boxes and plug in to the processor box the same way the temperature probes plug in to that box. The LOGGER understands several of the common interfaces used by microprocessors; OneWire, I2C and SPI. Serial ports are also available.

Currently available as standard plug in sensors are:

9.1 Analog to Digital conversion.

There is one A to D sensor built in to the LOGGER processor. In addition, the Analog to Digital plug in box adds eight more.

9.2 Digital Inputs and Outputs.

16 channels (pins) of I/O are available on each of two plug in boxes. 8 of these channels count pulses and can be used for liquid flow or kilowatt hours measurements.

9.2.1 Temperature and Humidity or Temperature Humidity and Atmospheric Pressure.

There is a plug-in box with a combination Temperature and Humidity sensor.

There is also a plug-in box with a combined Atmospheric pressure, Temperature and Humidity sensor.



9.3 Water Flow Measurement

This FS400A water flow sensor (and many others) can be plugged directly into the I/O modules of the LOGGER.



The conversion ratio from the pulses put out by the sensor to liters per minute are built in to the LOGGER. This ratio can be adjusted by the user on the Settings page. Gallons per minute are derived from the liters per minute conversion. Put a new multiplier or divisor in place for one of the pulse-

Using LOGGER for Food Temperature Monitoring
User Manual

counting pins. The  button must be pressed after each field is changed. If two or more fields are changed prior to pressing  all but one of the numbers changed will be forgotten.

Flow Pulse Counters (to get 1/100 liter per minute)		
lpmMultiplier_0	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_0	<input type="text" value="55"/>	<input type="button" value="Set"/>
lpmMultiplier_1	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_1	<input type="text" value="55"/>	<input type="button" value="Set"/>
lpmMultiplier_2	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_2	<input type="text" value="55"/>	<input type="button" value="Set"/>
lpmMultiplier_3	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_3	<input type="text" value="55"/>	<input type="button" value="Set"/>
lpmMultiplier_4	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_4	<input type="text" value="55"/>	<input type="button" value="Set"/>
lpmMultiplier_5	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_5	<input type="text" value="55"/>	<input type="button" value="Set"/>
lpmMultiplier_6	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_6	<input type="text" value="55"/>	<input type="button" value="Set"/>
lpmMultiplier_7	<input type="text" value="1000"/>	<input type="button" value="Set"/>
lpmDivisor_7	<input type="text" value="55"/>	<input type="button" value="Set"/>
<input type="button" value="Reboot"/>		



9.4 Power Consumption Measurement

Similar to computing fluid flow the LOGGER can compute Kilowatt Hour usage. Any pulse meter can be used. Good success has been achieved with a Wattnode Pulse meter from Continental Control Systems:



<https://ctlsys.com/product/wattnode-pulse/>

Connecting pins P1, P2, P3 of this meter directly to Pulse Counting pins of the LOGGER I/O module is all that is necessary (the COM pin connects to ground on the I/O module).

Similar to setting the flow count ratios the number of pulses per milliwatt is adjusted on the **Settings** page. Here too the button must be pressed after each field is changed. If two or more fields are changed prior to pressing all but one of the numbers changed will be forgotten.

KWH Pulse Counters		
mWatt_HR_per_Pulse_0	<input type="text" value="375"/>	<input type="button" value="Set"/>
mWatt_HR_per_Pulse_1	<input type="text" value="375"/>	<input type="button" value="Set"/>
mWatt_HR_per_Pulse_2	<input type="text" value="2500"/>	<input type="button" value="Set"/>
mWatt_HR_per_Pulse_3	<input type="text" value="2500"/>	<input type="button" value="Set"/>
mWatt_HR_per_Pulse_4	<input type="text" value="2500"/>	<input type="button" value="Set"/>
mWatt_HR_per_Pulse_5	<input type="text" value="2500"/>	<input type="button" value="Set"/>
mWatt_HR_per_Pulse_6	<input type="text" value="10000"/>	<input type="button" value="Set"/>
mWatt_HR_per_Pulse_7	<input type="text" value="10000"/>	<input type="button" value="Set"/>

10 Future Capabilities

The Dragonnorth Group is constantly improving the LOGGER features. Some of these features show up in the LOGGER when only part of the capability is completed.

10.1 Text Alerts

Sending Alerts by text messages is a planned future capability.



11 Advanced Features

Many advanced features are controlled on the Settings page. This page is called Permanent Variables at the top because the value of these settings is remembered when power to the LOGGER is shut off. The values are also remembered when the LOGGER reboots.

Internally the LOGGER counts some times in milliseconds. These counts turn into negative numbers after about 25 days and wrap around after about 50 days. To keep from getting confused the LOGGER automatically reboots when the millisecond counts become too large (every 25 days).

11.1 Choosing Engineering Units

Some sensors present values in engineering units that people understand, Volts, degrees, liters and gallons are examples of engineering units. For some values the LOGGER can be told what type of units to present.

11.1.1 Centigrade vs Fahrenheit

The presentation of temperatures can be in degrees Centigrade or degrees Fahrenheit. On the Settings page click the appropriate button to change the units.

← → ↻ 🏠 🔒 Not secure | 192.168.12.179/parameters.html?signature=Mikey ☆ 🐼 ⋮

Permanent Variables

Basics
[Home](#)
[Sensor Values](#)
[Version](#)
Sensor History
[All Sensors](#)
[Humidities](#)
[Temperatures](#)
[Voltages](#)
Exports
[XML](#)
Output Control
[I/O Pin Control](#)
Sensors by Name
[Named Periods](#)
Setup and Configuration
[Database](#)
[Email SMTP Setup](#)
[Data Map](#)
[M2X Setup](#)
[Security](#)
[Network Setup](#)
[Sensor Configuration](#)
[Settings](#)
[Get Time \(manually\)](#)
[Temperature Sensors](#)
[Time History](#)
[Update Firmware](#)
[Get NTP Time](#)

Network Status
Running as: Access Point AND Server
After Reboot run as: Access Point AND Server


Units
Temperature Units ☐ F ☒ C


Permanent Parameters
PERM_VERSION 1
PERM_SIZE 598
SSID_NAME
SSID_PASSWORD
CONFIG_MODE 3
MINIMUM_PULSE_LENGTH
Deep Sleep after each sample ☒ ON ☐ OFF
Pulse counting will not work if turned ON.

KWH Pulse Counters
mWatt_HR_per_Pulse_0
mWatt_HR_per_Pulse_1
mWatt_HR_per_Pulse_2
mWatt_HR_per_Pulse_3
mWatt_HR_per_Pulse_4
mWatt_HR_per_Pulse_5
mWatt_HR_per_Pulse_6
mWatt_HR_per_Pulse_7



11.2 Database Control

Samples are taken at a periodic rate and stored in a file on the SD card. The periodic rate is set when the file is first created and cannot be changed. Changing the **Seconds Between Samples** effects the next time a database file is created. Emptying the database file will lose all data. If a new sampling rate is desired the recommended procedure is to set the new sampling rate by putting the number of seconds between samples in the field and press the  button. Then remove power from the LOGGER and remove the batteries. Put in a new blank SD card and restore power to the LOGGER. The database file on the new card will use the new sampling rate. Preserve the old card as a backup of your previous sample history.

It is possible to tell the LOGGER to empty the database by putting DESTROY in the field and pressing the  button. This is dangerous since all previous samples will be lost.

The LOGGER can display samples at any desired interval, there is no need to slow down the sampling rate to display samples at a longer interval. The only reason to change the sampling rate is to save power when the LOGGER is used in Battery Operation. See the



Battery Operation Section for details about putting the LOGGER to sleep between samples.

Database Control

Basics Home Sensor Values Version Sensor History All Sensors Humidities Temperatures Voltages Exports XML Output Control I/O Pin Control Sensors by Name Named Periods Setup and Configuration Database Email SMTP Setup Data Map M2X Setup Security Network Setup Sensor Configuration Settings Set Time (manually) Temperature Sensors Time History Update Firmware <input type="button" value="Get NTP Time"/>	For database Creation SecondsBetweenSamples <input type="text" value="10"/> <input type="button" value="Set"/> Note: SecondsBetweenSamples is part of the database. Once a database is created it can not be changed. The value set here will get used when a new database is created. The recommended method is to set this value then to turn off the LOGGER and insert a new SD card. The database created on the new SD card will use the SecondsBetweenSamples sample interval. The sensor history is kept in a database on the SD card. Deleting this database will lose the entire sample history . Instead of deleting the database consider using a new SD card and keeping the old one as an archive. <input type="text"/> Input 'DESTROY' and click the button to clear the database and start over. <input type="button" value="Empty the Database"/> <input type="button" value="Reboot"/>
---	---



11.3 Email Alerts

Sending email alerts when a sensor gets out of range is feature of the LOGGER. In order to send emails you must have an SMTP account that is capable of sending emails from the IP address where the LOGGER is located. For spam security protection most ISPs have security issues that prevent email from sending from the LOGGER. Dragonnorth Group gets around this issue by using an account at <https://www.smtp2go.com/>. The server port account and password are set to values associated with that account.

11.3.1 Set up SMTP Server

Once you have an account that is capable of sending email from a 'remote' location set up the SMTP email account on this page and use the button to verify that the LOGGER is capable of sending emails.

Email Configuration

Basics Home Sensor Values Version Sensor History All Sensors Humidities Temperatures Voltages Exports XML Output Control I/O Pin Control Sensors by Name Named Periods Setup and Configuration Database Email SMTP Setup Data Map M2X Setup	<h3>Email Alerts Configuration</h3> <table><tr><td>SMTP_SERVER</td><td><input type="text" value="mail.smtp2go.com"/></td><td><input type="button" value="Set"/></td></tr><tr><td>SMTP_PORT</td><td><input type="text" value="2525"/></td><td><input type="button" value="Set"/></td></tr><tr><td>SMTP_ACCOUNT</td><td><input type="text" value="your account"/></td><td><input type="button" value="Set"/></td></tr><tr><td>SMTP_PASSWORD</td><td><input type="text" value="your password"/></td><td><input type="button" value="Set"/></td></tr><tr><td>EMAIL_FROM</td><td><input type="text" value="sender@yourdomain.com"/></td><td><input type="button" value="Set"/></td></tr><tr><td>EMAIL_TO</td><td><input type="text" value="you@yourdomain.com"/></td><td><input type="button" value="Set"/></td></tr></table> <div><input type="button" value="Send Test Email"/></div> <div><input type="text" value="0"/> <input type="button" value="Set Time Between Alerts"/></div> <p>When a value goes out of range an email and/or text is sent. To prevent a great number of alerts from being sent once an alert is sent additional alerts will not be sent for this period. A value of 0 turns off email alerts.</p>	SMTP_SERVER	<input type="text" value="mail.smtp2go.com"/>	<input type="button" value="Set"/>	SMTP_PORT	<input type="text" value="2525"/>	<input type="button" value="Set"/>	SMTP_ACCOUNT	<input type="text" value="your account"/>	<input type="button" value="Set"/>	SMTP_PASSWORD	<input type="text" value="your password"/>	<input type="button" value="Set"/>	EMAIL_FROM	<input type="text" value="sender@yourdomain.com"/>	<input type="button" value="Set"/>	EMAIL_TO	<input type="text" value="you@yourdomain.com"/>	<input type="button" value="Set"/>
SMTP_SERVER	<input type="text" value="mail.smtp2go.com"/>	<input type="button" value="Set"/>																	
SMTP_PORT	<input type="text" value="2525"/>	<input type="button" value="Set"/>																	
SMTP_ACCOUNT	<input type="text" value="your account"/>	<input type="button" value="Set"/>																	
SMTP_PASSWORD	<input type="text" value="your password"/>	<input type="button" value="Set"/>																	
EMAIL_FROM	<input type="text" value="sender@yourdomain.com"/>	<input type="button" value="Set"/>																	
EMAIL_TO	<input type="text" value="you@yourdomain.com"/>	<input type="button" value="Set"/>																	



Using LOGGER for Food Temperature Monitoring

User Manual

11.3.2 Set Sensor Limits

Sensor limits can be set up at any time. It makes the most sense to set them up after email is properly configured and tested. The limits are stored in a file on the SD card called `sensoralerts.bin`. Also stored in this file is the time between alerts. Each time new limits are set the new value is appended to the file. The time that the limits were set is also logged in the file. The file is read when the LOGGER boots and the last entry in the file is used. When a sample is taken the sensor value is checked to see if the value falls between the Min and Max values for that sensor. An Alert email is sent when the sensor value is first observed outside that range. Another email will not be sent until the number of minutes between alert has elapsed.

Basics
[Home](#)
[Sensor Values](#)
[Version](#)

Sensor History
[All Sensors](#)
[Humidities](#)
[Temperatures](#)
[Voltages](#)

Exports
[XML](#)

Output Control
[I/O Pin Control](#)

Sensors by Name
[Named Periods](#)

Setup and Configuration
[Database](#)
[Email SMTP Setup](#)
[Data Map](#)
[M2X Setup](#)
[Security](#)
[Network Setup](#)
[Sensor Configuration](#)
[Settings](#)
[Set Time \(manually\)](#)
[Temperature Sensors](#)
[Time History](#)
[Update Firmware](#)
[Get NTP Time](#)

System Status
WiFi Name: **LOGGER_6b03**
Time since boot: **54**
Number of reboots: **113**

Sensor Configuration

Alerts are sent by text and/or email when the sensor value is less than the minimum or greater than the maximum. Set both to 0 to turn off alerts.

Each time the name of a sensor is changed (Set New Name) the time and new name is logged. At system startup this list is read and the most recent name is used.

Name	Information	Settings
A	0.741 V Uses 12 bits Unique ID: 1afe34d26b030000 Device: Processor ADC pin Datatype: Voltage 3 decimal places Sensor specific data: 17	<input type="text"/> Set New Name Min Max <input type="text"/> 0.000 <input type="text"/> 0.000 Set New Limits
Temperature_0	25.37 C Uses 16 bits Unique ID: 103a80530208007b Device: DS18x20 Datatype: Degrees C 2 decimal places Sensor specific data: 0	<input type="text"/> Set New Name Min Max <input type="text"/> 0.00 <input type="text"/> 10.00 Set New Limits

96 sensors (124 allowed) with 94 disabled. 95 bytes (754 bits) of sensor data.

[Set Minutes Between Alerts](#)

When a value goes out of range an email and/or text is sent. To prevent a great number of alerts from being sent once an alert is sent additional alerts will not be sent for this period.
A value of 0 turns off email alerts.

[Erase User Sensor Names](#)

Input 'ERASE' and click the button to clear the user defined sensor names.
Pressing this button will erase the entire history of user name setting. A reboot is necessary to revert to the default names.

[Erase Email and Alerts](#)

Input 'ERASE' and click the button to clear the Min/Max alerts.
Pressing this button will erase the entire history of alerts. A reboot is necessary to eliminate all alerts.

[Reboot](#)



Using LOGGER for Food Temperature Monitoring User Manual

11.4 Battery Operation

The LOGGER is capable of running on batteries. It will run several days on three AA cells. If longer battery life is desired the LOGGER can be configured to collect samples and sleep between samples to save power. The LOGGER will run for about a year when taking a sample every 10 minutes and sleeping between samples. NOTE: While sleeping the LOGGER will not respond as a Web Browser. Also while sleeping the LOGGER does not count pulses thus it will not record water flow, pulse counts or kilowatt hour usage.

Go to the settings page and configure the LOGGER to “Deep Sleep after each sample”. The LOGGER will stop responding to your browser a short time once this is done.

Once it has started sleeping to wake the LOGGER up disconnect any USB power and take out the batteries. When power is restored the LOGGER will stay awake for several minutes and the web pages can be used normally. Every time a web page is read or refreshed this time is reset and the LOGGER will stay awake for another few minutes. Turn off sleeping to keep it awake if desired.

← → ↻ 🏠 ⓘ Not secure | dragonnorth.com:256/parameters.html ☆ 🧑

Permanent Variables

Basics
[Home](#)
[Sensor Values](#)
[Version](#)
Sensor History
[All Sensors](#)
[Humidities](#)
[Temperatures](#)
[Voltages](#)
Pin History
[Pulse Counts](#)
[Kilowatt Hours](#)
[RPM](#)
[Water \(gpm\)](#)
[Water \(lpm\)](#)
Exports
[XML](#)
Output Control
[I/O Pin Control](#)
Sensors by Name
[Named Periods](#)
Setup and Configuration
[Database](#)
[Email SMTP Setup](#)
[Data Map](#)
[M2X Setup](#)
[Security](#)
[Network Setup](#)
[Sensor Configuration](#)
[Settings](#)
[Set Time \(manually\)](#)
[Temperature Sensors](#)
[Update Firmware](#)
[Get NTP Time](#)


Network Status
Running as: Access Point AND Server
After Reboot run as: Access Point AND Server
Units
Temperature Units ☐ F ☒ C
Permanent Parameters
PERM_VERSION 1
PERM_SIZE 598
SSID_NAME
SSID_PASSWORD
CONFIG_MODE 3
MINIMUM_PULSE_LENGTH
Deep Sleep after each sample ☐ ON ☒ OFF
Pulse counting will not work if turned ON.
KWH Pulse Counters
mWatt_HR_per_Pulse_0
mWatt_HR_per_Pulse_1
mWatt_HR_per_Pulse_2
mWatt_HR_per_Pulse_3
mWatt_HR_per_Pulse_4
mWatt_HR_per_Pulse_5
mWatt_HR_per_Pulse_6
mWatt_HR_per_Pulse_7
Flow Pulse Counters
(to get 1/100 liter per minute)
lpmMultiplier_0
lpmDivisor_0
lpmMultiplier_1
lpmDivisor_1



11.6 Security

The LOGGER has a simple signature-based security scheme. There are two signatures (passwords), one for reading data and another for making changes. When the signatures are blank any request is allowed. If the read signature is set and the write-signature is not the read signature must be supplied to make changes.

Once a signature is set every web page request must also supply the signature. An example link is provided on the Security Configuration page. After setting a signature be sure and bookmark this link to be able to access the LOGGER in the future.

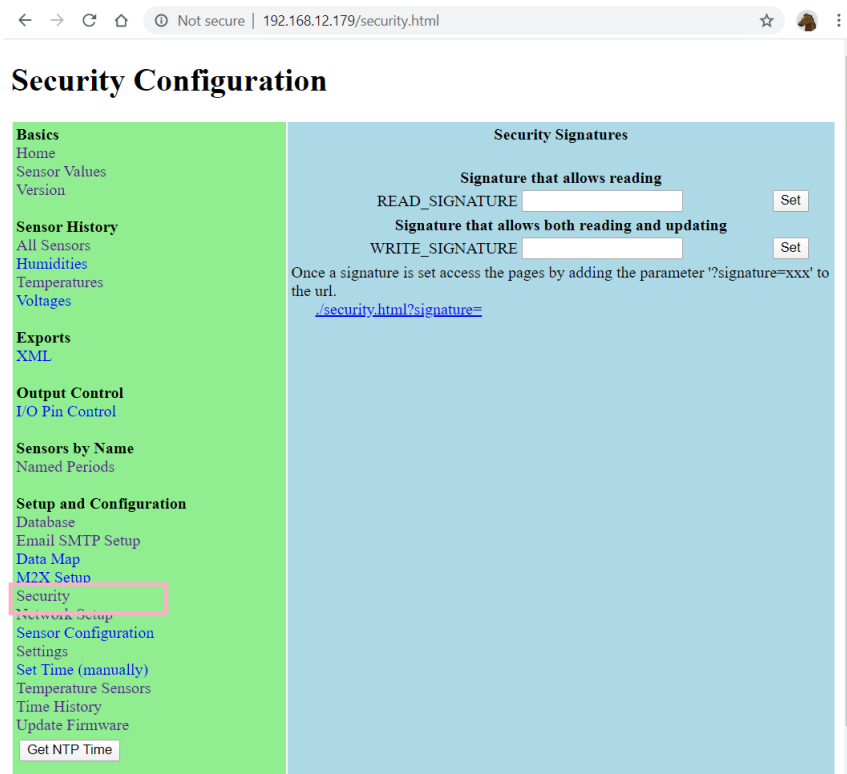

← → ↻ ⌂ Not secure | 192.168.12.179/security.html ☆

Security Configuration

Basics
Home
Sensor Values
Version

Sensor History
All Sensors
Humidities
Temperatures
Voltages

Exports
XML

Output Control
I/O Pin Control

Sensors by Name
Named Periods

Setup and Configuration
Database
Email SMTP Setup
Data Map
M2X Setup
Security
Network Setup
Sensor Configuration
Settings
Set Time (manually)
Temperature Sensors
Time History
Update Firmware
Get NTP Time

Security Signatures

Signature that allows reading

READ_SIGNATURE

Signature that allows both reading and updating

WRITE_SIGNATURE

Once a signature is set access the pages by adding the parameter '?signature=xxx' to the url.

[./security.html?signature=](/security.html?signature=)

11.7 Exporting Data

XML is a standard way of transferring data between computers on the Web. LOGGER supports reading sample data in XML format. This can be used by computer programs to read data from the LOGGER and

Using LOGGER for Food Temperature Monitoring User Manual

can also be used by creating the XML data in your browser and saving the file. The history.xml link on this page is an example for a computer program. The [Get XML Data](#) button.

XML Request

Basics
Home
Sensor Values
Version

Sensor History
All Sensors
Humidities
Temperatures
Voltages

Exports
XML

Output Control
I/O Pin Control

Sensors by Name
Named Periods

Setup and Configuration
Database
Email SMTP Setup
Data Map
M2X Setup
Security

XML data can be read by reading history.xml with arguments
startTime=# (a UNIX time_t)
count=# number of samples requested
interval=# number of seconds between samples

[history.xml?startTime=0&count=2&interval=10](#)

will read the latest sample and the sample from 10 seconds ago.

Set the time and number of samples and press a button.

Start (GMT): - - : :

Samples:

Seconds between:

[Get XML Data](#)


Current Time: 17-May-2020 19:53:58 GMT
Configuration is: OK from database
Database starts at: 3-May-2020 1:05:14 GMT
Database ends at: 17-May-2020 19:53:14 GMT
Last Sample: 17-May-2020 19:53:14 GMT
Next Sample Due: 17-May-2020 19:55:14 GMT



12 Time Synchronization

When connected to the internet the LOGGER automatically updates time from **pool.ntp.org** servers, the same time servers that most computers use. These time servers in turn keep time synchronized with the time services provided by the National Institute of Standards: <https://www.nist.gov/pml/time-and-frequency-division/time-services>.

Pressing the “Get NTP Time” button:



Tells the LOGGER to fetch a time update from these time servers. There are rules about how often a time update can be performed so the LOGGER may not be able to immediately comply with the request.

When the internet is not available the LOGGER gets time from its internal clock chip. The clock chip is updated periodically from the internet when that becomes possible.

The LOGGER records time to the nearest second. While connected to the internet times logged by a LOGGER can be expected to be within two seconds of the NIST standard. Most of the time they will be within one second of that standard.

Without the internet the LOGGER will maintain time to within 2 minutes per month at 25 degrees C. This is based on the clock chip (a Maxim DS2417) specification.

Battery powered systems read time from the internal time chip. This will have a drift in time of up to 2 minutes a month as noted above.

13 Data Storage

Several files are kept on the SD card inserted into the logger.

The SD card uses a normal file system and can be plugged into any computer to copy the data for backup purposes.

File	Purpose
datalog.bin	History of all sensor readings.
namehistory.bin	A report of names for periods of data.
timehistory.bin	A report of when the LOGGER adjusted the clock.

The LOGGER reads sensors and creates a permanent record of what it has observed. This data is stored in the file called datalog.bin. The frequency of sampling is user adjustable, but can be changed only when a new datalog.bin file is created which destroys all of the previous data. By default, the LOGGER reads all sensors every 10 seconds and stores that data on the SD card. At that sampling rate a 32Gb card will store at least 20 years of data.

Reading the sensors less often is desirable only if the LOGGER will be battery powered. Reading four temperature sensors every 10 minutes should be able to run for a year on three AA batteries. Note that



Using LOGGER for Food Temperature Monitoring User Manual

running on batteries requires special configuration and that a LOGGER does not act as a web server when configured for long life running on batteries.

As the LOGGER fills the SD card with data access to the file slows down. The symptom of this is that pages will be slower to display. The slowdown is most noticeable when reading hundreds of samples over a long period (i.e. a sample each day for a year). This effect can be observed after a year or two of data has been accumulated. The slowdown is due to fragmentation of the space on the SD card. Periodically copying the data to a new SD card will restore the speed of the LOGGER. It is recommended that this be done at least once a year. The old SD card becomes a backup of your data.


Performance will also be restored if you copy the file to a computer, quick format the SD card, and copy the data back. It is believed that a simple copy of the file to a computer deletion of the file on the SD card and copying the file back will also restore the speed, but, this has not been verified.



14 Troubleshooting

14.1 Missing Database

This indication appears on many pages including the Sensor Values page when the SD card is missing or has a problem.

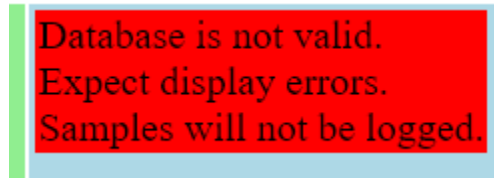

Check that the SD card is inserted and insert a good SD card if necessary.

14.2 Can Not See the LOGGER

One of the most common problems is that the LOGGER is no longer visible on your network. The first thing to do is to power cycle the LOGGER (be sure and remove the batteries too the LOGGER will not turn off until both USB power and the batteries are disconnected).

If power cycling the LOGGER does not help try connecting to the LOGGER using the LOGGER as your WiFi network (see section 3.1.1 Connect to the LOGGER). It is possible that the LOGGER has forgotten your WiFi network name and password.